

## Specification

Filtration · Rapid Tests · Water Analysis · Chromatography · Bioanalysis  
Filtration · Schnellteste · Wasseranalytik · Chromatographie · Bioanalytik


Product:	CHROMAFIL® Polyamide (PA) / Nylon
REF:	729048
	Filters are HPLC certified for low level UV-absorbing substances for gaining accurate chromatographic results
Housing material:	Polypropylene (PP)
Colour code:	top: yellow bottom: green
Membrane filter material:	Polyamide (Nylon)
Pore diameter:	0.20 µm
Filter diameter:	15 mm
Filtration area:	~ 1.6 cm <sup>2</sup>
Pressure stability:	> 12 bar
Connections inlet:	Female luer lock
Connections outlet:	Minispike
Dead volume:	~ 35 µL

## HPLC-test


Conditions:	Two mL of the solvent (specified under the chromatograms) were applied to the filter; 100 µL of the filtrate were injected to the HPLC.
Eluent A:	water
Eluent B:	acetonitrile
Gradient:	10% 95% B in 25 minutes
Flow rate:	0.5 mL/min
Sensitivity:	-5 to 10 mAU at 254 nm
Column:	125/4 NUCLEODUR® C18 Gravity 5 µm (REF: 760100.40)

# Specification


Filtration · Rapid Tests · Water Analysis · Chromatography · Bioanalysis  
Filtration · Schnellteste · Wasseranalytik · Chromatographie · Bioanalytik

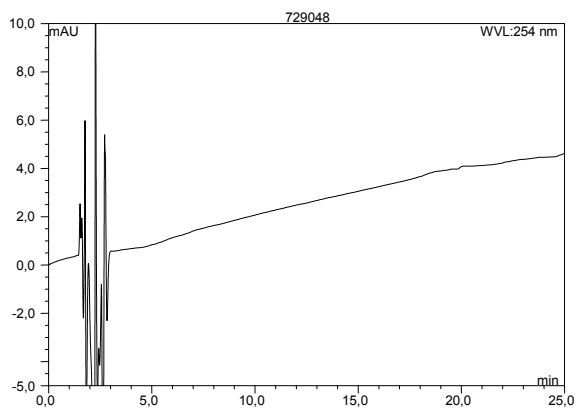

Methanol filtrate

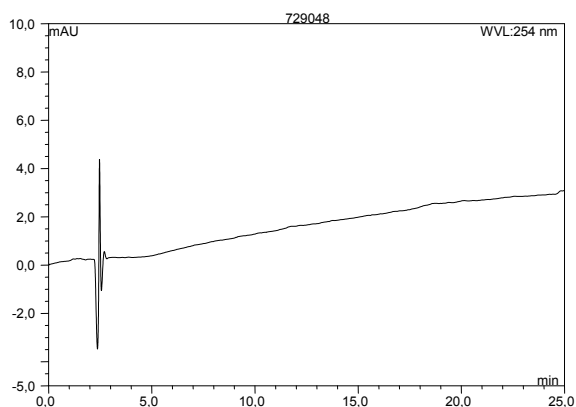

Water filtrate

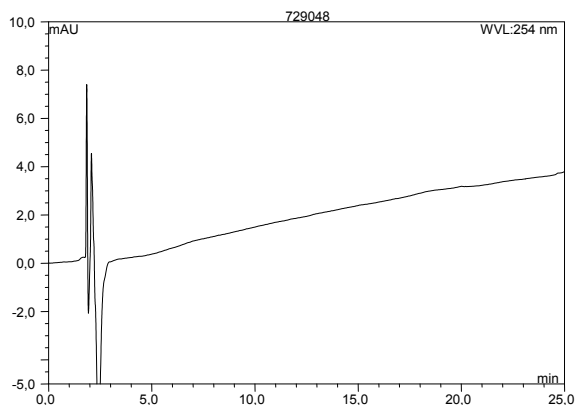

Acetonitrile filtrate